


Processing Method:	Derivati PhNCO_2	Project Name:	Interesterifikacija\Deriv PhNCO
Processing Method ID:	1545	System:	Massspek
Channel:	234.0nm	Calibration ID:	1546
Proc. Chnl. Descr.:	****		
Date Calibrated:	1/23/2019 5:06:48 PM EET		

A 1.316935e+005
 B 4.775760e+008
 C 0.000000e+000
 D 0.000000e+000
 R^2 0.999960

Calibration Plot

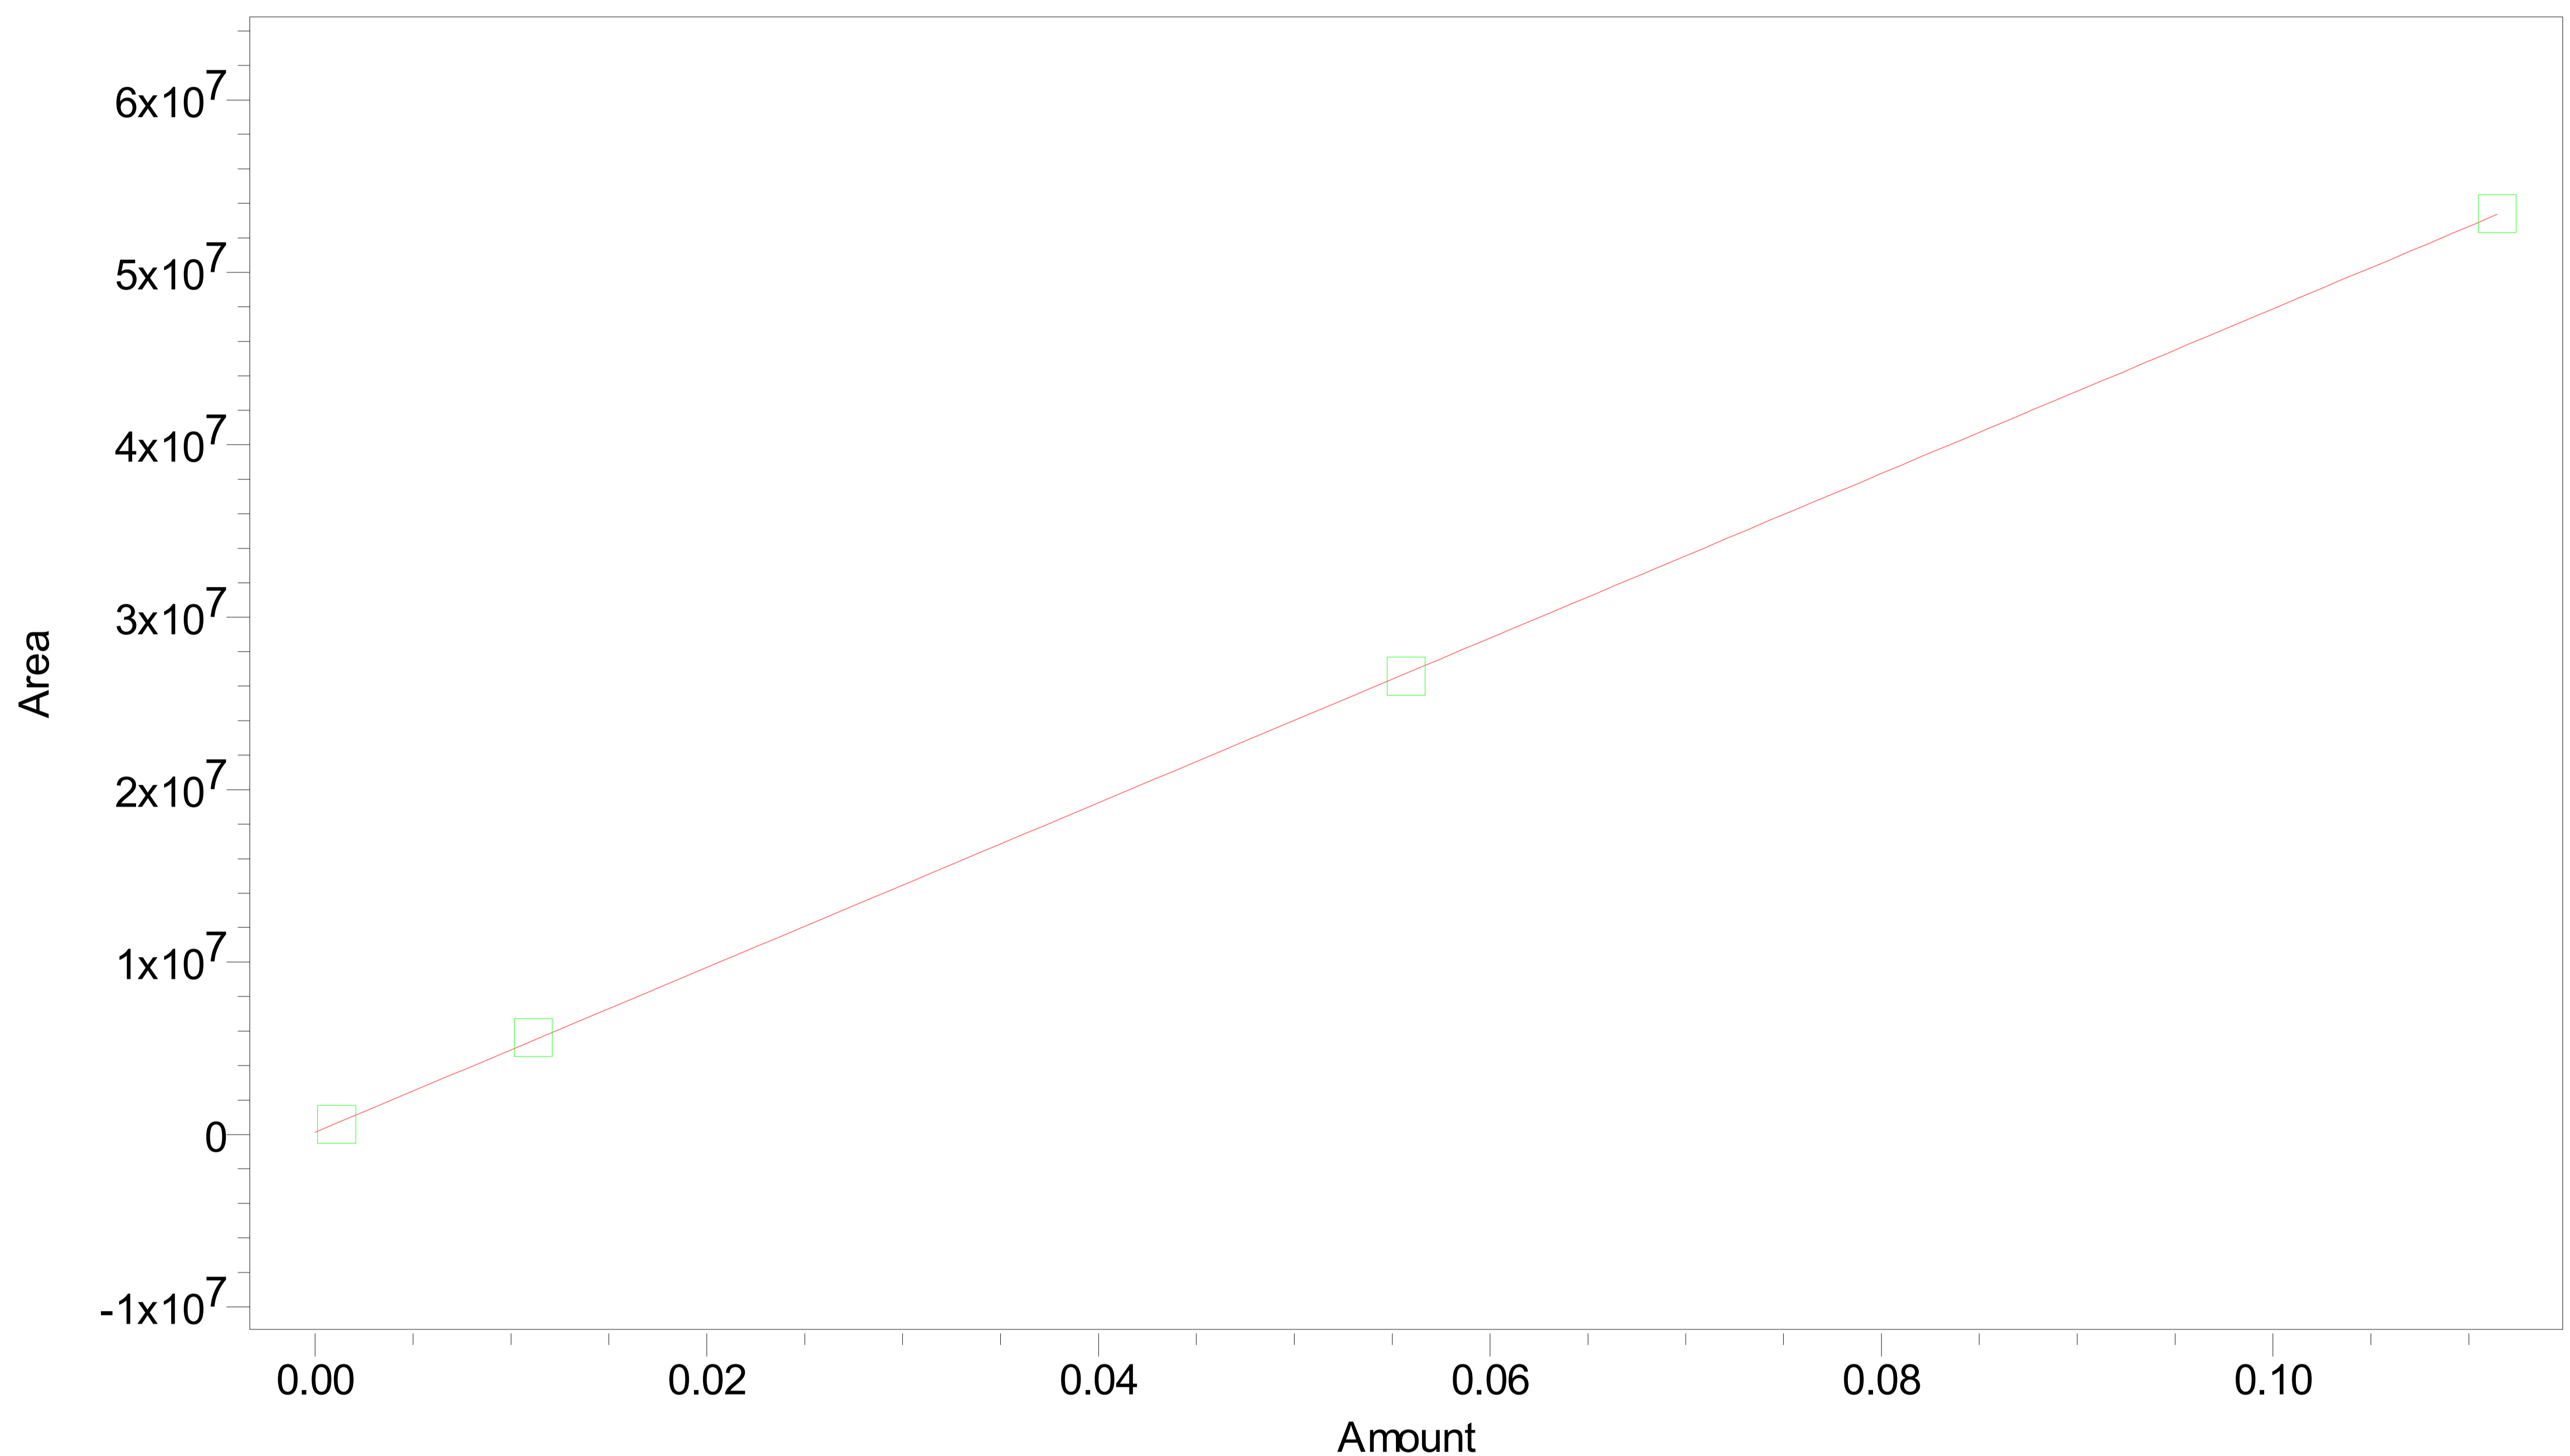

Peak: DFG

	Name	Level	X Value	Response	Calc. Value	% Deviation	Manual	Ignore
1	DFG	2-100	0.001114	581624.348677	0.000942	-15.430	Yes	No
2	DFG	2-10	0.011145	5634251.818684	0.011522	3.381	Yes	No
3	DFG	2-0.5	0.055724	26582726.506855	0.055386	-0.607	Yes	No
4	DFG	2-1	0.111449	53420593.866782	0.111582	0.119	Yes	No