


Processing Method:	Derivati PhNCO_2	Project Name:	Interesterifikacija\Deriv PhNCO
Processing Method ID:	1545	System:	Massspek
Channel:	234.0nm	Calibration ID:	1546
Proc. Chnl. Descr.:	****		
Date Calibrated:	1/23/2019 5:06:48 PM EET		

A 1.595010e+005
 B 1.137090e+009
 C 0.000000e+000
 D 0.000000e+000
 R^2 0.999882

Calibration Plot

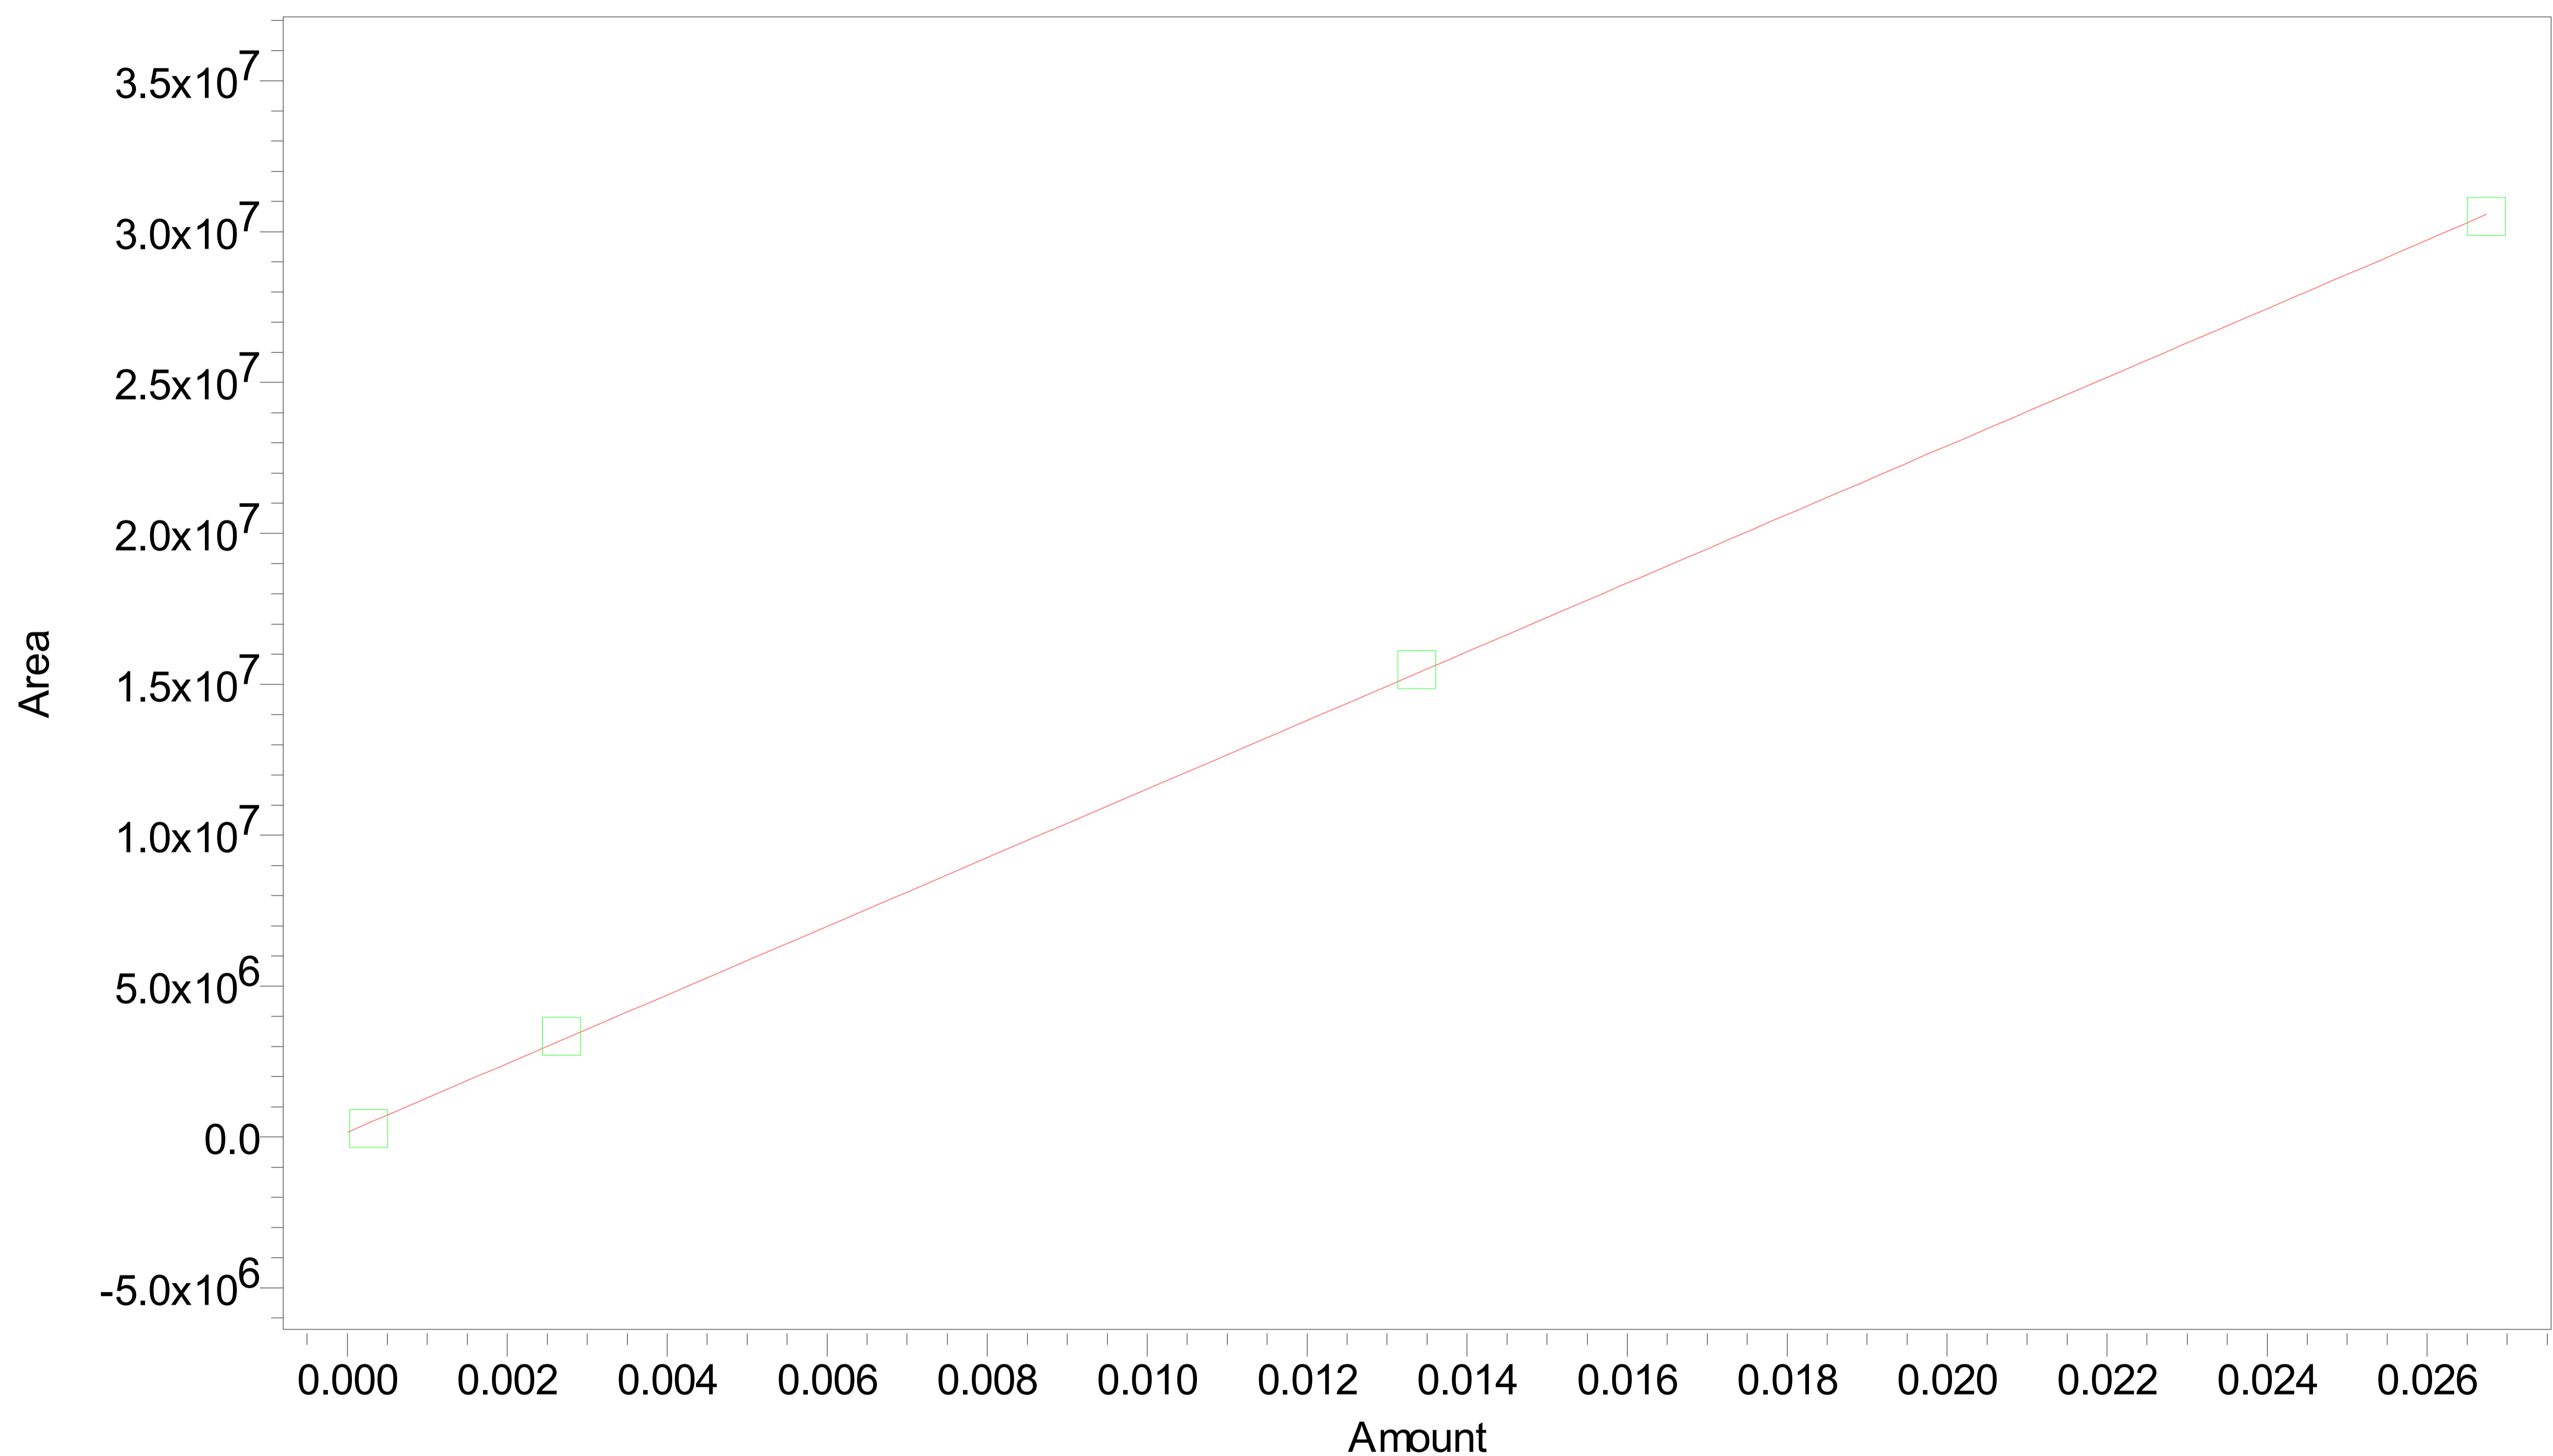

Peak: MFG

	Name	Level	X Value	Response	Calc. Value	% Deviation	Manual	Ignore
1	MFG	2-100	0.000267	286035.514674	0.000111	-58.322	Yes	No
2	MFG	2-10	0.002675	3330827.945136	0.002789	4.261	Yes	No
3	MFG	2-0.5	0.013373	15483112.691301	0.013476	0.771	Yes	No
4	MFG	2-1	0.026745	30501114.711146	0.026684	-0.230	Yes	No