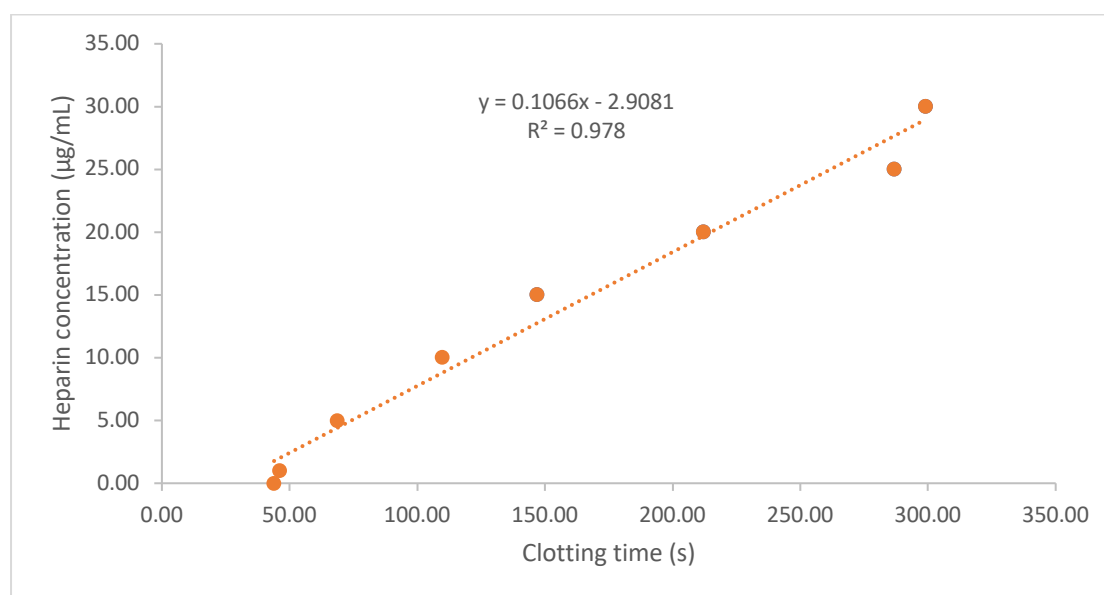


<b>Code</b>	<b>Conc. %</b>	<b>Conc. µg/mL</b>	<b>N1</b>	<b>N2</b>	<b>N3</b>	<b>N4</b>	<b>AVER.</b>
H1	0.0030	30.00	319.52	303.92	295.32	277.36	299.03
H2	0.0025	25.00	290.56	290.36	259.28	306.20	286.60
H3	0.0020	20.00	185.32	201.20	202.16	259.04	211.93
H4	0.0015	15.00	151.64	141.76	139.86	154.16	146.86
H5	0.0010	10.00	97.52	117.52	116.16	107.72	109.73
H6	0.0005	5.00	67.76	68.56	65.84	72.00	68.54
H7	0.0001	1.00	46.76	46.52	46.00	44.92	46.05
Milli-Q	0.0000	0.00	43.68	43.52	44.28	44.25	43.93



**Fig. S1. Prepare a calibration curve of heparin**